


CERTIFICATION OF ANALYSIS


Product Name	Bacteriostatic Water	Lot Number	AYK20260515-BAC10
Appearance	Clear, colorless liquid	Laboratory ID	LB20260515-027
Main Component:	Sterile Water with 0.9% Benzyl Alcohol	Manufacturing Date	2026/5/12
Specification	10ml/vial	Report Date	2026/5/15

HPLC CHROMATOGRAM

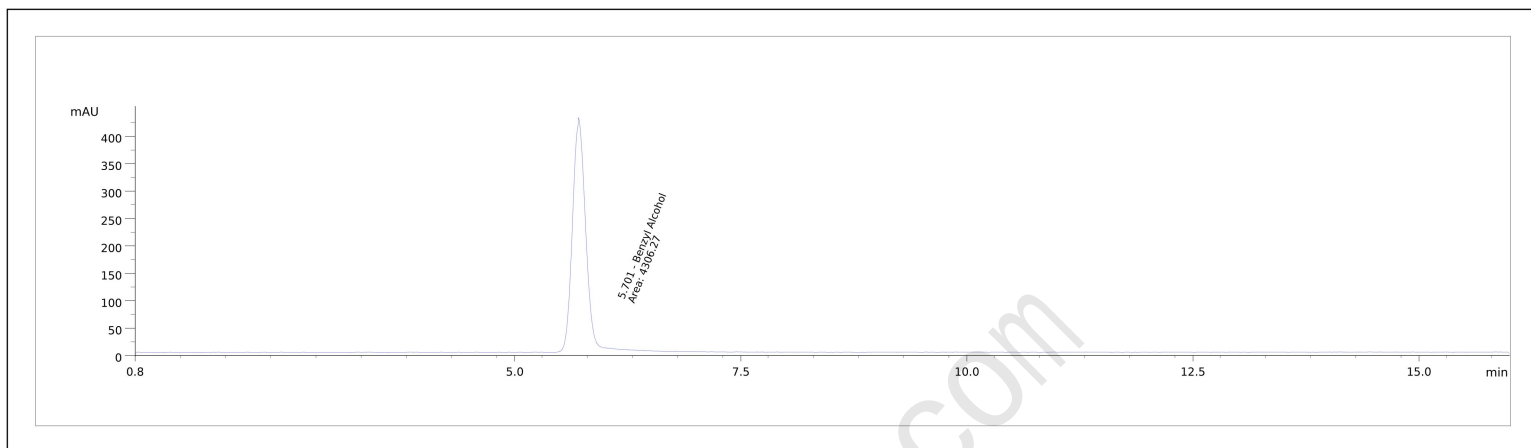

MASS IDENTIFICATION

Inten.(x10,000)

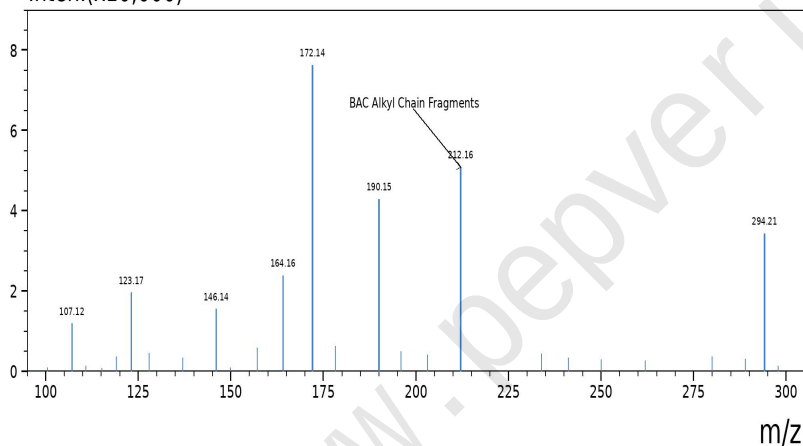

PRODUCT IMAGE



ANALYSIS RESULTS

Specification	Result	Method	Status
Identity:BAC Water	Positive for Benzyl Alcohol	HPLC -UV	✓ Conforms
Content	0.91%w/v	HPLC Quantitation	✓ Conforms
pH	5.84	pH Meter	✓ Conforms

NOTES & DISCLAIMER

The analytical testing reported herein was conducted under controlled laboratory conditions using validated HPLC and LC-MS methodologies. The results presented are specific to the tested batch and may be influenced by storage conditions, sample handling, transportation, and other experimental variables. This certificate is intended for research and quality verification purposes only.

Analyzed By: wang kun
2026/05/15

Approved By: HUANG YU
2026/05/15